


Humidity Generation and Calibration Equipment

**THUNDER SCIENTIFIC**  
**CORPORATION** THE HUMIDITY SOURCE

# Model 2500

## Flow Meter Removal Procedure

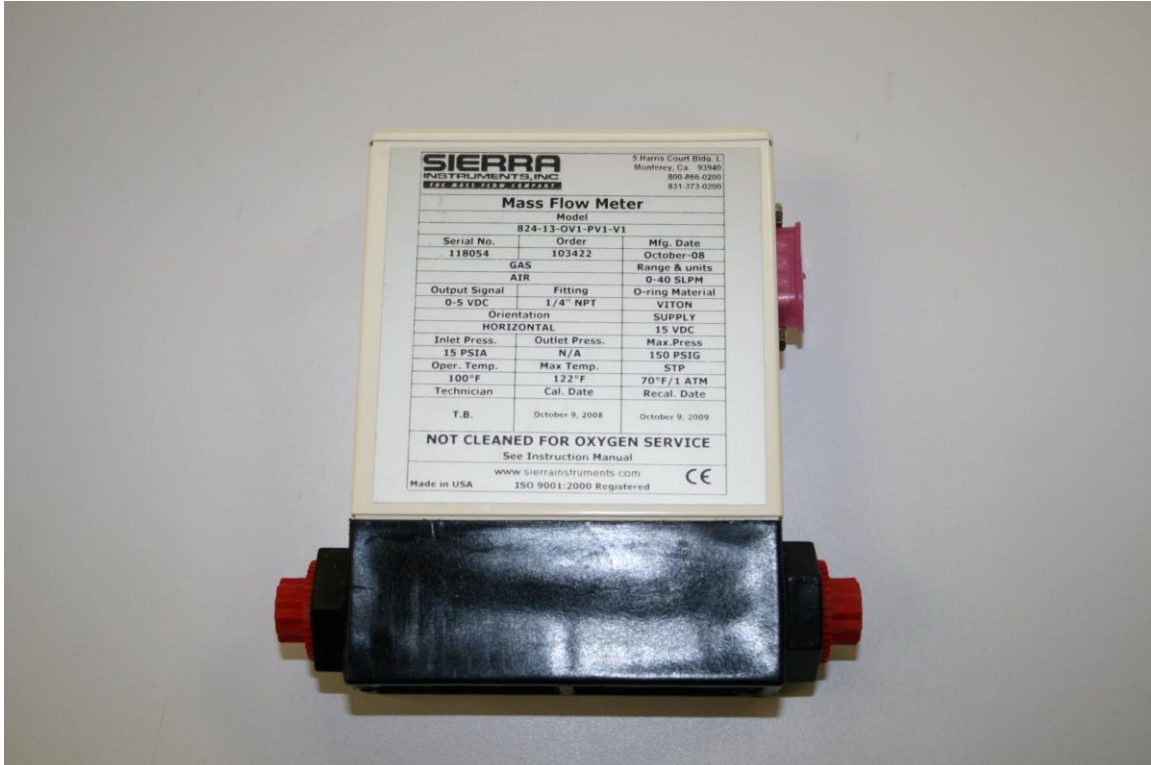

Tech Support Document TSD-0202  
Revision Date: October 20, 2009

623 WYOMING BLVD. SE



ALBUQUERQUE, NM 87123-3198  
[WWW.THUNDERSCIENTIFIC.COM](http://WWW.THUNDERSCIENTIFIC.COM)



TEL: 505.265.8701  
FAX: 505.266.6203