

Humidity Generation and Calibration Equipment

THUNDER SCIENTIFIC
CORPORATION THE HUMIDITY SOURCE

Model ACS-517B

Hose Replacement Specifications



Tech Support Document TSD-0221
Revision Date: July 14, 2009

623 WYOMING BLVD. SE



ALBUQUERQUE, NM 87123-3198
WWW.THUNDERSCIENTIFIC.COM




TEL: 505.265.8701
FAX: 505.266.6203

Hose replacement specifications

Hose must be rated for at least 100 °C / 200 psi.

Length of the hose, not including fittings is 10.25" and the I. D. of the hose is 3/8".

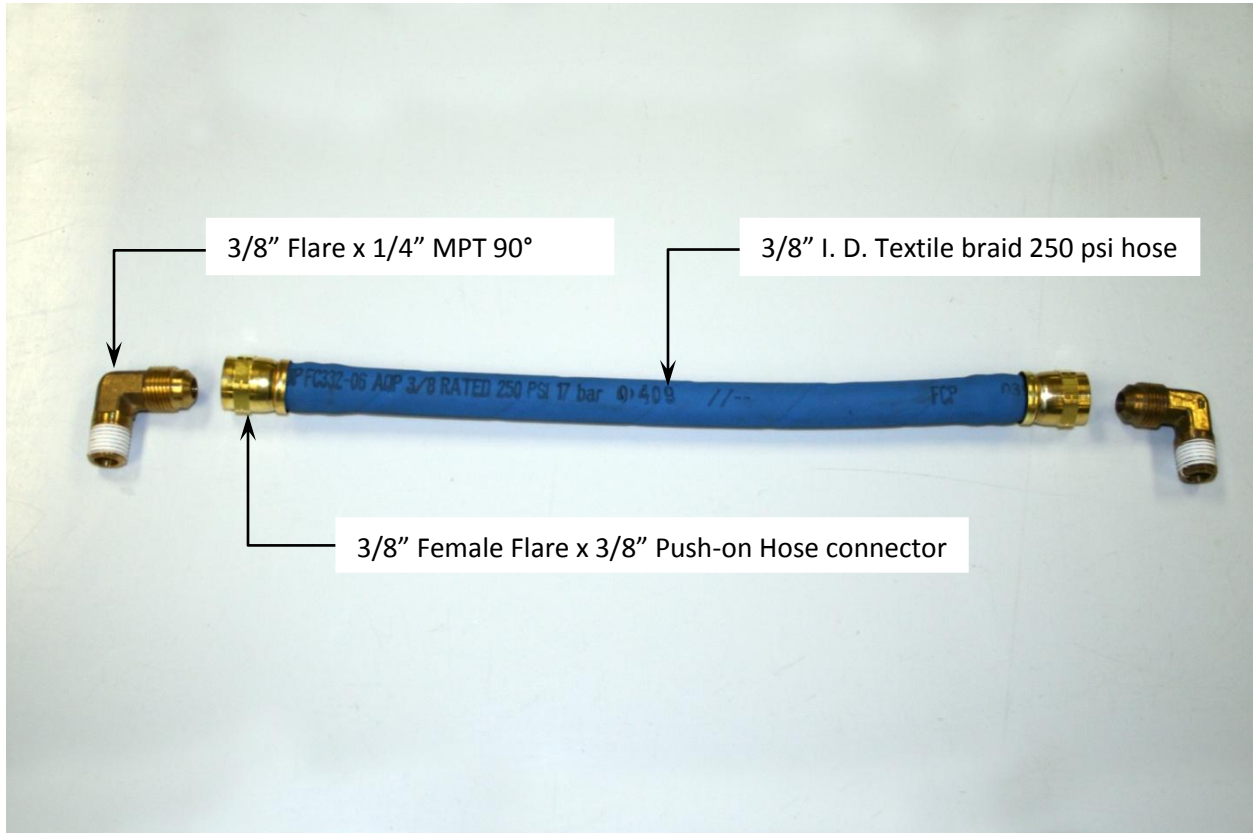


Use two each of the 3/8" Flare x 1/4" MPT 90° Elbows, part number (A337).

Use two each of the 3/8" Female Flare x 3/8" Push-on Hose connectors, part number (G5A246).

Use Eaton/Aeroquip hose part number (FC332-06).

This hose replacement is for the Thomas® compressor part number (TA-5172).

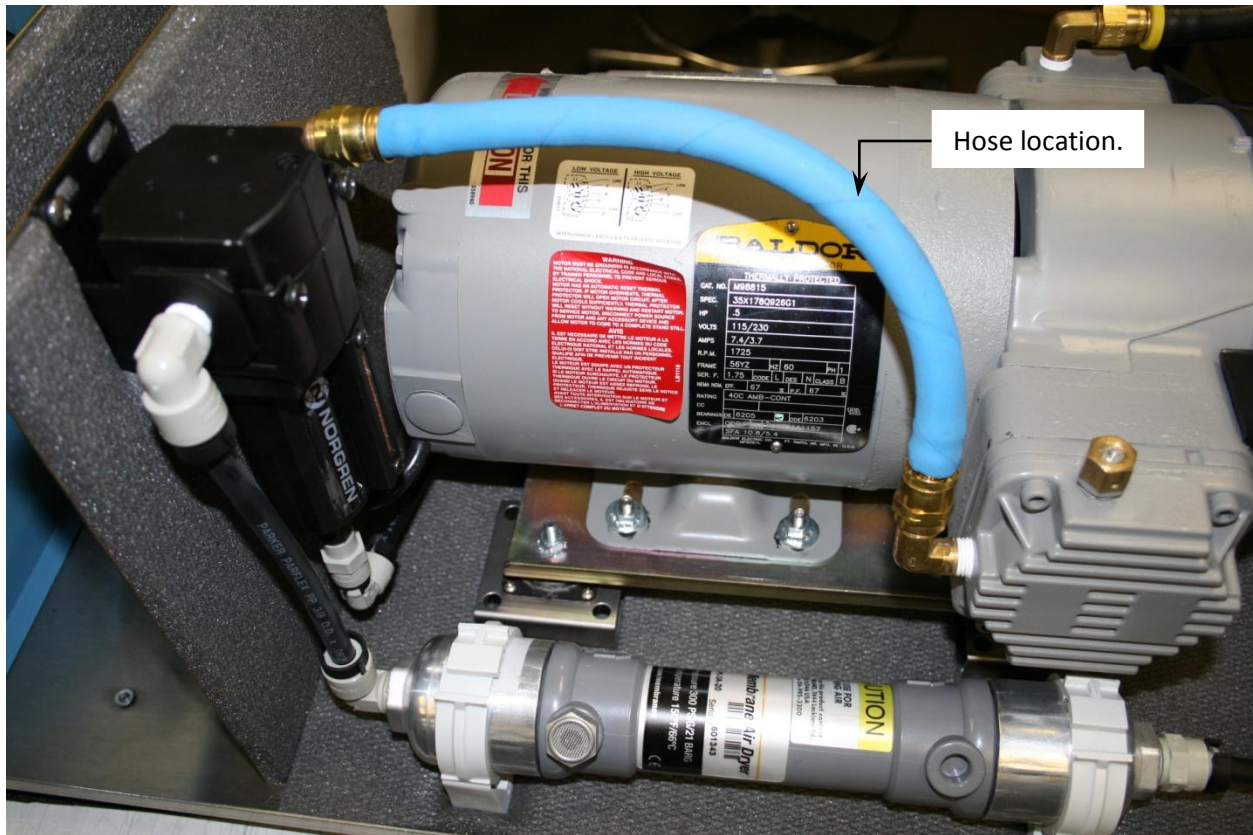

Insert the hose in this location.

Should you have any questions, contact Thunder Scientific at 1-800-872-7728 or, E-mail support@thunderscientific.com.